



## LaMotte Tracer PockeTester

### LaMotte Tracer PockeTester Basics

The LaMotte meter has three measurements modes:

- 1) Conductivity
- 2) Total dissolved solids (TDS)
- 3) Salinity

You will need to cycle through the three modes when using the meter by pressing and holding the MODE button. The ALLARM Shale Gas Volunteer Monitoring Protocol uses the meter to test for conductivity and TDS.

Calibrate your meter at home every time before going streamside to monitor.



- If you monitor several sites in one day, calibrate the meter only once on that day.
- If you monitor several sites over several days, calibrate the meter every day before you monitor.
- When performing dual calibration, calibrate the low range first, keep the meter on and then do the middle range.

### Step #1: Calibrate the Meter –Dual Calibration (home)

- (A) Turn the meter on – press the **ON/OFF** button.
- (B) Take the cap covering the electrodes off.
- (C) Set the meter to conductivity mode –  $\mu\text{S}$  will be displayed above the reading (see diagram for symbols). To change modes, press and hold the **MODE** button until it switches modes (~2 seconds), then immediately release the button. Repeat until  $\mu\text{S}$  is displayed on the screen.  
*Tip: If the meter enters the “hold” mode, press the mode button to exit.*
- (D) Shake the bottle of 84  $\mu\text{S}/\text{cm}$  calibration solution and pour ~20 mL of solution into the calibration vial.

*When doing dual calibration, you must start with low range 84  $\mu\text{S}/\text{cm}$ , keep the meter on, and then do the middle range 1413  $\mu\text{S}/\text{cm}$ .*

- (E) Place the electrode into the solution, and allow the reading to stabilize. This may take up to two minutes.
- (F) Once the reading is stable, press and hold the **CAL** button for ~3 seconds, until **CAL** appears on the bottom of the screen and **84** flashes. When the meter has been calibrated, **SA** and **End** will briefly flash and the meter will return to the conductivity measurement mode. **SA** will not flash if the calibration fails.
- (G) Rinse the electrode with distilled water and shake dry.
- (H) Repeat steps C-G with the **1413  $\mu\text{S}/\text{cm}$**  calibration solution.
- (I) Make a note on your data sheet that you calibrated your meter – step #4 on the ALLARM Chemical and Stage Monitoring Data Sheet.

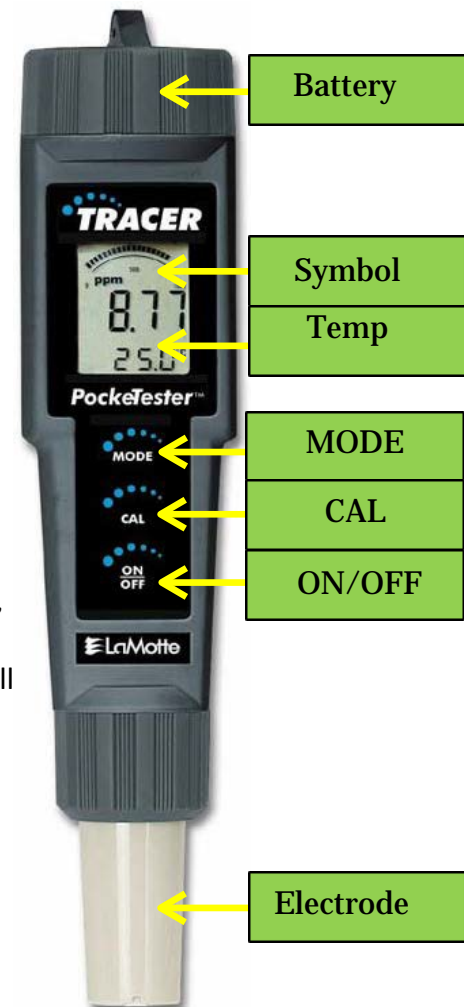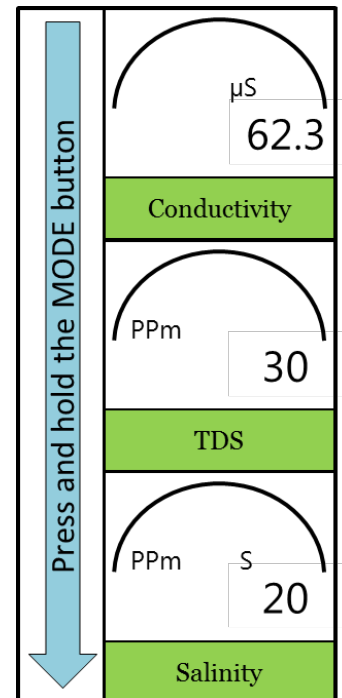

### Step #2: Measure Conductivity (stream-side)

- (A) Turn the meter on – press the **ON/OFF** button.
- (B) Take the cap covering the electrodes off.
- (C) Set the meter to conductivity mode – **μS** will be displayed above the reading (see diagram for symbols). To change modes, press and hold the **MODE** button until it switches modes (~2 seconds), then immediately release the button. Repeat until **μS** is displayed on the screen.
- (D) Place the electrode into the water so that it is fully covered – directly into either the stream or your stream testing bottle. Allow the reading to stabilize. This may take up to two minutes.

*If you use a stream testing bottle to gather your measurements, shake the bottle before placing the meter in the water.*

Instructional videos can be found on ALLARM's YouTube page, [https://www.youtube.com/channel/UCWzeO\\_3CtrsF8XbL2dCw8Q](https://www.youtube.com/channel/UCWzeO_3CtrsF8XbL2dCw8Q). Visit ALLARM's Shale Gas Monitoring Toolkit for additional monitoring resources at [ALLARMwater.org](http://ALLARMwater.org).

- (E) Record the conductivity measurement on your data sheet.

### Step #3: Measure Total Dissolved Solids (stream-side)

- (A) **Without removing the meter from the water**, change the meter to total dissolved solids mode. Press and hold the **MODE** button for ~2 seconds – **TDS** will flash on the bottom of the screen and **ppm** will be displayed above the reading.
- (B) Allow the reading to stabilize.
- (C) Record the total dissolved solids measurement on your data sheet.

*Ppm and mg/L are used interchangeably*

### Step #4: Replicates & Wrap-up (stream-side)

Repeat steps #2 and #3 to measure the second replicate for each parameter.

- (A) Press and hold the **MODE** button to switch from TDS to salinity.
- (B) Press and hold the **MODE** button to change from salinity to conductivity mode (**μS** will be displayed above the reading).
- (C) Record the second conductivity and TDS result on your data sheet.
- (D) Average the two replicates for each parameter and record the average value on your data sheet.

*Round the average of your TDS values to the nearest multiple of ten.  
Ex: 110 ppm (mg/L) + 120 ppm (mg/L) / 2 = 115 ppm (mg/L) → 120 ppm (mg/L)*

- (E) Rinse the meter with distilled water, shake dry, and turn the meter off – press the **ON/OFF** button.

## Troubleshooting the LaMotte Tracer PockeTester

If you are having difficulties calibrating or using your meter, try the following options:

<b>Reset the meter</b>	<b>Replace the batteries</b>
<ol style="list-style-type: none"><li>1. Turn the meter off.</li><li>2. Simultaneously press the ON/OFF, CAL, and MODE buttons momentarily. "dFlt" will be displayed on the screen.</li></ol>	<p>The batteries in the PockeTester will need to be replaced every 2-5 years, depending on use. There is a low battery indicator on the meter that displays "BAT" when the batteries become weak. You can find replacement batteries (CR2032) at any local box/grocery/home improvement store or online. Four new batteries cost ~\$2. To replace batteries: turn off the meter, open the battery compartment cap, remove battery carrier by pulling on the two black plastic outer tabs on the battery carrier. Observe polarity of batteries (a diagram is located on the side of the battery carrier) and replace batteries, then replace battery carrier and battery compartment cap.</p>

For additional help troubleshooting your meter, contact ALLARM.